



# Vitality Enhancement System

## Instruction Guide

## Table of Contents

Disclaimer .....	3
Introduction .....	3
The <i>IonCleanse</i> System .....	4
Contraindications .....	4
<i>IonCleanse</i> Front Panel .....	5
Quick Start Instructions .....	6
Increasing Conductivity .....	8
Incorporating Minerals .....	9
Alarm Messages .....	9
Recommended Usage and Settings .....	11
Frequency and Time of Sessions .....	11
What to Expect from a Session .....	12
Colors and Objects in the Water .....	12
Regional Toxicity .....	13
Ionization Potential .....	14
Smudging .....	14
How the <i>IonCleanse</i> Works .....	15
Generating Ions .....	15
The Meaning of Positive and Negative .....	15
Care of your <i>IonCleanse</i> unit .....	16
Marketing your <i>IonCleanse</i> service .....	16
Muscle Testing .....	17
Nutritional Protocols .....	18
Metal Plate Replacement .....	21
Limited Warranty Information .....	23
Metal Plate Replacement Log .....	25

## Disclaimer

Thank you for incorporating the *IonCleanse*<sup>®</sup> Vitality Enhancement System into your health maintenance program. As you were advised when you purchased this unit, the *IonCleanse* is not intended to treat, prevent, cure, or diagnose any disease.

The IonCleanse Vitality Enhancement System is a comprehensive health and wellness system and the information provided by A Major Difference is solely for use as a part of a self-improvement program. None of the information provided is intended to act as a substitute for medical counseling, nor does it involve the diagnosis, prognosis, or prescription of remedies for the treatment or prevention of any disease.

Please read this manual carefully before you start *IonCleanse* sessions. The information it contains will help you understand the science behind the unit and enable you to effectively answer most client questions. Everyone is different, and the *IonCleanse* system can be adjusted to accommodate 99.5 percent of the population. However, because overuse can decrease energy levels, please follow the instructions and proceed carefully for optimum results.

## Introduction

The *IonCleanse* Vitality Enhancement System includes a footbath, homeopathics, and specialized food supplements, along with a pulsed laser for accelerating toxin release. The homeopathics, food supplements and laser are purchased separately. Used properly, the IonCleanse system provides a comfortable and relaxing way to rid the body of toxins and rejuvenate aging organs and glands.

## The *IonCleanse* Vitality Enhancement System

Today, we are exposed to the greatest toxic load in the history of our planet, and ongoing periodic cleansing is essential to maintain health and to avoid disease. The *IonCleanse* system, in combination with a healthy, low-stress lifestyle, provides a thorough and efficient way to maintain high energy levels and long term wellness.

It may be possible to improve comfort and well-being despite a lifetime of toxic buildup in the body. The long-term effectiveness of the *IonCleanse* Vitality System depends on other life-enhancing changes that the client is willing to make.

## Contraindications


Any person falling into one or more of the categories listed below should not use the *IonCleanse*:

- Wearer of a pacemaker or any other battery operated or electrical implant.
- Patients or clients who do not respond to a muscle test, or who test weak to both polarities with their feet in the water and with the unit turned on.
- Those on heartbeat regulating medication.
- Organ transplant recipients.
- Organ removal, especially the colon. Great care should be exercised when dealing with patients or clients who have had organs removed as their bodies do not function at high energy levels. Colon removal indicates a greatly impaired ability to process nutrients and remove toxins from the body.
- Anyone on medication, the absence of which would mentally or physically incapacitate them, such as psychotic episodes, seizures, etc.

Furthermore, the following recommendations should be strongly considered:

- Many medications require that a blood level be maintained in order to be effective, for example, blood pressure medication. Try to schedule an *IonCleanse* session just before the taking of a medication so that the patient or client can maintain proper blood levels of their medication.
- Great care should be taken with reluctant or overly skeptical patients or clients who are suffering from pathologies and are under the allopathic care system. These individuals do not understand the alternative healing paradigm and are not prepared to undergo the rigors of detoxification.
- Patients with low blood sugar should eat before receiving a session. The *IonCleanse* tends to lower blood sugar in diabetics and may do so with those who are hypoglycemic.
- It is best not to bathe pregnant women and breast-feeding mothers because the *IonCleanse* system pulls toxins out of tissues and fat that **could** impair fetal development and **will** become part of the milk that is fed to a newborn infant.
- Use your professional judgment in working with clients on dialysis, taking insulin, or experiencing congestive heart failure. Gentle detoxification can help the body to eliminate the toxins that the kidney and heart cannot eliminate on their own and will not interfere with medications or deplete insulin levels.
- You can probably work with people who have a metal joint implant, but some have found the exposure to an electromagnetic field to be uncomfortable. In the event of discomfort, stop the session immediately.
- If you are ever in doubt or have questions regarding the use of the *IonCleanse* with a patient or client, contact Bob Moroney toll free at 877-315-8638 for assistance before bathing.

## IonCleanse Front Panel

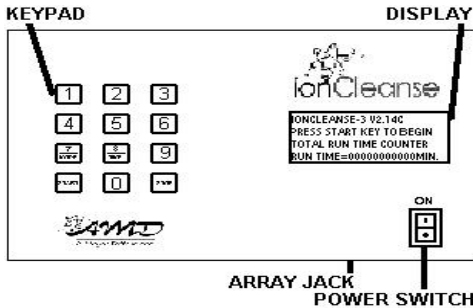

## Quick Start Instructions

### To Prepare the IonCleanse For Use

1. Plug the array's permanently attached cord in the front of the IonCleanse unit.
2. Plug the power supply unit into the back of the main unit and then into an outlet.
3. Place the array upright in, or hook it to the side of, a plastic container holding 3-4 inches of water. Be sure that the copper tube at the center of the array is covered with water. **Important note: Do not cover the top of the array with water. If you submerge the top of the array in the water, the nuts, washers and connectors will corrode and your unit will not function properly.**
4. Have the patient immerse feet in the water and turn on the unit.
5. Press the "start" key.

## Quick Start Instructions (cont.)

6. Press “7/Mode” to step through the five polarity options until the desired option is displayed (see Polarity Options below).
7. When the desired option is displayed, press “8/Time” to select option.
8. Key in desired session duration in minutes (1 – 60). Entering more than 45 minutes will trigger a warning.

### Polarity Options

The *IonCleanse* comes preset with five polarity options. However, if you are a layperson, or you are not familiar with muscle testing, **we strongly recommend that you use only option 3** (the 70+ / 30– option), which has been developed for use without muscle testing.

The following describes the five preset options and recommended use:

1. All Positive – Clinicians only.
2. All Negative – Clinicians only.
3. 70+ (positive) / 30– (negative). This is the generic setting that should be used by non-clinicians and those who do not muscle test for one polarity or another.
4. 15+ (positive) / 10– (negative) / 5+ (positive)
5. 10– (negative) / 15+ (positive) / 5– (negative)

**Note:** Options 4 and 5 were developed over thousands of sessions. We have found that people who test for positive polarity first generally require option 4; those who test for negative polarity first generally require option 5. Therefore, in most cases where patients test for positive, use option 4; for those who test strong in negative, use the option 5.

## Manual Polarity Override

To manually override positive polarity output to the array, press 4 while the unit is running; to manually override negative polarity output to the array, press 5.

## Keypad Description

Other special keypad options are:

0 puts the unit into diagnostic mode

8 puts the unit into demonstration mode

“Start” begins the polarity options or the programs

“Stop” pressed on either digit of the time entry returns the unit to the “Select Treatment Program” menu. If you hold the “Stop” key for 2 – 3 seconds right after entering the time, or when the “Time preset to 30 minutes” message is displayed, the unit will return to the “Program the Array Polarity” menu.

## Increasing Conductivity

Regardless of where you are in the country, the *IonCleanse* removes all guesswork as to the amount of salt you should add in order to increase conductivity. For our purposes, conductivity relates to the water’s ability to transmit a small amount of electricity.

All types of water, with the exception of distilled water, have some degree of conductivity. The conductivity of the water determines the amount of ionization potential, which in turn determines the effectiveness of the session. If the unit shows less than 1.8 amps, add a small amount of salt to the water in order to raise the water’s conductivity. **Important note: Add as little salt as possible to the water in order to maximize the life of the array. The less corrosive material in the water, the longer the metal plates will last.** The optimum operating range of the *IonCleanse* unit is between 11-24 volts, and 1.8–2.50 amps. Both of these readings are displayed during an *IonCleanse* session. A reading below 11 volts will not produce more power, but will generate more heat in the unit.

## Incorporating Minerals

We believe that some people can lose electrolytes (calcium, potassium, sodium, and magnesium) during *IonCleanse* sessions. If you are a layperson, make sure that you are taking a good vitamin supplement that provides those minerals, along with fatty acids and vitamin C. Because detoxification accelerates change in the body, these supplements help to support this process.

## Alarm Messages

The unit is in constant self-diagnosis and shows a variety of messages to warn of error conditions on the four-line display panel:

### SYSTEM SHUTDOWN! OUTPUT OVERLOAD!

The machine has detected an overload in the power output to the array. Amperage exceeding 2.50 amps indicates a hardware failure in the control box. The message is displayed, an audio tone sounds, and the unit shuts off automatically.

### OVER TEMPERATURE FAN COOL FAILURE

The machine has detected that the power unit has overheated. A current below 1.00 amps with a voltage of less than 8.00 volts indicates a cooling fan or array output overload, resulting in this failure alarm message and an audio tone. The unit shuts off automatically. Ensure that the vents are clear and turn on again. Try fresh water with no salt.

### POWER PACK FAIL! VOLTAGE TOO HIGH!

The machine has detected a power pack failure, that the wrong power pack is plugged into the machine, that the voltage regulator in the external power pack has failed, or that the normal 24-volt supply voltage has exceeded 29.5 volts for some reason. The message displays, a tone sounds and the unit shuts off.

ARRAY NOT IN H2O OR SALT REQUIRED  
VOLTAGE =           , CURRENT =

If no load is detected on the array 30 seconds after power is supplied to the array, the unit displays the error message, alternating every three seconds with the actual voltage and current readings. This alarm can indicate one of the following conditions:

- a. Array is not in water.
- b. Water is insufficiently conductive, such as when distilled water is used. Add a small amount of salt and stir it into the water. Then check the amperage and voltage readings to make sure they change when the array is in the water. With the array in the water, normal current range is 1.8 – 2.50 amps, and normal voltage range is 11 – 24 volts.
- c. The array cable is not plugged into the control box.
- d. The array cable has a broken wire in the plug, in the cable or in the array connection.
- e. The control box has developed an internal failure or broken wire.

### **Demo Mode**

To enter demo display, hold the 8 key while switching the machine on. (To quit this mode, you must power the unit off.)

### **Diagnostic Mode**

To enter the diagnostic mode, hold the 0 key while switching on. Enter the diagnostic password 4802.

### **Diagnostic Mode Key Functions**

Press the following keys to test the unit's internal functions.

- |                              |                                    |
|------------------------------|------------------------------------|
| 1 fan on, array on           | 6 sound test low                   |
| 2 fan off, array off         | 7 show output volts and amps       |
| 3 negative polarity to array | 8, 9, 0, start, stop key test only |
| 4 positive polarity to array |                                    |
| 5 sound test high            |                                    |

## Recommended Usage and Settings

You can use the *IonCleanse* unit with anyone over two years of age, as long as you supervise the sessions and follow the Quick Start instructions. However, the recommended time and frequency will vary from person to person. Children's sessions take considerably less time than adults' sessions. (see below)

### Frequency of Sessions: Use Clinical Judgment

As a general rule, the maximum session frequency for clients under 50 years of age is once every other day for 14 sessions, with a three-week break before beginning the next sequence of 14 sessions. Use clinical judgment as everyone is different. Client fatigue requires a reduction in treatment time and an increase in session spacing.

The maximum recommended session frequency for those over 50 is once every third day, with a two-week break after 14 sessions.

The following considerations are for doctors and clinicians only:

- Persons with chronic conditions can consider bathing every other day without a break, as long as they don't lose energy or become uncomfortable.
- Children with autism can consider bathing every other day without a break.
- Without the benefit of muscle testing, 30-minute sessions are the recommended maximum time for adults, and 15 minutes or less for children under 10 years of age.

If your patient feels tired after a session or reports feeling angry, panicky, etc., space the sessions further apart and check for mineral depletion. Fatigue indicates an overstressed condition, and emotional upheaval indicates that emotional toxins are being released along with chemical toxins.

## What to Expect from a Session

Healthy individuals can expect to feel lighter and experience a greater feeling of well being from each *IonCleanse* session.

## Colors and Objects in the Water

Many colors and objects will appear in the water during *IonCleanse* sessions as a result of the reaction between the toxins and particles in the water, any salt added to the water, the metals in the array, and the acidity or alkalinity of your patients. All of these combine to produce color, **even though no feet are in the water**. The color produced by these reactions depends on the water's toxic and chemical impurities in your geographic area.

Water is all around us, from the air we breathe, to the water we bathe in, to the water that we drink and use for cooking. All this water forms one unified field. Because our bodies are approximately 70% water, we ourselves interact with this field. The toxins in our bodies will look similar to the toxins predominant in a specific area; however, there will be more toxic particles in the water with the patient's feet immersed. You will also find that the water-based toxins will not stick to the side of the bucket and array, whereas substances coming out of the body will form a sticky ring that must be removed with a detergent or scouring powder.

Despite similarities due to toxicity of the water in a particular geographical area, we note that specific patients' detoxification processes will tend to determine the water color. Based on EAV (Electro Acupuncture by Voll) testing, the following table (Fig. 1) shows what we believe the colors in the water to represent.

We have also seen parasites, pinworms, and smelly purple mucous coming from patients on medication for dairy allergies. If you operate more than one unit in your office, you may need an ionizer to neutralize the various odors patients give off.

Fig .1

<b>Color or particle</b>	<b>Material of area of the body being detoxified</b>
Yellow-green	Kidneys, bladder, urinary tract, female/prostate area
Orange	Joints
Brown	Liver, tobacco, cellular debris
Black	Liver
Dark green	Gallbladder
White foam	Mucous from lymph system
White cheese-like particles	Most likely yeast
Black flecks	Heavy metals
Red flecks	Blood clot material

### Regional Toxicity

Water, metal and salt will combine to produce color and objects in the water even without feet in the container. The *IonCleanse* will neutralize toxins in the water the same way it neutralizes toxins in the body. The predominant color of the de-ionized water is determined by the chemicals used by the local water authorities, in combination with the pollutants common to that area. In Denver, Colorado, for example, the predominant water color is orange; in Phoenix, Arizona, orange-brown; in parts of Texas, brown; and in Boise, Idaho, yellow-green.

Chinese acupuncturists understand the concept of regional toxicity as it relates to the ailments that predominate in a given area. Some areas of the country have higher joint complaints, while others report higher frequencies of kidney/bladder problems. Could it be that the toxins peculiar to an area gravitate to a specific part of the body and cause it to break down?

As a general rule, regional toxins contribute 20 – 40 percent of the residues found in the water after a footbath. Any black flecks can be created by heavy metals in the water as well as deterioration of the metal in the array. Experience and the observations discussed above

will help you determine what is coming from the patient and what is coming from the array. They are distinctly different.

The greater the concentration of active minerals in the water, the greater the ionization potential of the water. Chlorine, fluorine, and the new chlorine neutralizers (used by water authorities to mask chlorine—see note below) greatly reduce the ionization potential of the water because they bond with the ions produced by the *IonCleanse*, thus neutralizing them.

### Ionization Potential

A growing number of municipal water systems appear to be using highly chlorinated water with a masking agent that neutralizes the taste and smell of the chlorine. You will be able to recognize this water because your patient's bath water will only turn a pale yellow-green, and you will detect a strong chlorine odor from it. That odor emanates from the ions being generated from the *IonCleanse* attempting to neutralize the highly toxic water. This type of water cannot be used with the *IonCleanse* because the combination of chlorine and neutralizing agent also neutralizes ion exchange activity as well. You should get a different array of colors and objects in the water from each session. If you get a consistent pale green color over several sessions, try switching to distilled or chlorine-free spring water and add more mineral salt to the water in half-teaspoon increments.

### Smudging

Smudging is the burning of a clump or cluster of sage in a room. This process is used to clean a room of odors and psychic debris. Because people dump psychic and physical debris during *IonCleanse* sessions, you may want to consider using a smudging process to cleanse the bathing area.

To use the smudging process, simply light a cluster of sage and fan it throughout the room and into each corner. You can also use a room ionizer to clean the room of odor, but not psychic debris.

## How the *IonCleanse* System Works

### Generating Ions

The array goes into the water with the hands, feet, or body, and the control unit delivers a small direct current into the array, which causes the metals within the array, in combination with the water and salt, to generate positively and negatively charged ions by separating the water into oxygen and hydrogen.

The ions generated by the *IonCleanse* create an osmotic field that pulls neutralized toxins out of the body through that portion of the skin that is in contact with the water.

### The Meaning of Positive and Negative

For the purpose of *IonCleanse* discussions, positive and negative relate to electrical, rather than chemical phenomena.

When the *IonCleanse* is set on positive, the current is being directed to the positive pole in the array, which results in more negative ions being produced in the water. Therefore, positive polarity generates a negative ion flow, which, we believe, raises blood pH from acidic toward alkaline. An ion is a charged atom that has gained or lost an electron, and creates a magnetic field capable of neutralizing oppositely charged particles. These neutralized particles are pulled out of the body through the skin via a process called **osmosis**, or the movement of particles through a membrane, from a lower concentration to a higher concentration. In this case, the higher concentration is the ion field set up by the array in the water.

## Care of Your *IonCleanse* Unit

The array housing is made of acrylic, which will attract and hold sludge from the baths. Clean your array between each session with a disinfectant such as kitchen/bathroom cleaner, grapefruit seed extract, or vinegar. We recommend that you soak your array in an ascorbic solution every 5-10 sessions to remove any excess corrosion. Please see instructions on sample bag.

The lifetime of your array will vary depending on the amount of chlorine and fluorine in the water, and the acidity of your patients. Because corrosion rates vary widely across the country, we cannot guarantee the number of sessions that you will get from a set of plates.

Call us at 303-755-0112 or toll free at 877-315-8638, or visit our website at: [www.amajordifference.com](http://www.amajordifference.com) for the up-to-date price of new arrays and plates.

**Important note: If you submerge the array during *IonCleanse* sessions, the connectors will corrode and the array will not produce the correct voltage or current.**

## Marketing Your *IonCleanse* System

Your *IonCleanse* system is the best show-and-tell device ever developed to demonstrate the build-up of toxic odors and substances that lodge in the human body. If you already have a busy practice, simply offer every patient a free session and, if they find it beneficial, suggest a sequence of 10 – 14 sessions. It's just as easy to sell a sequence as it is to sell one session.

Do not make claims other than improved patient comfort and the possible health benefits of cleansing in general. Just keep putting people's feet in the water - most people love the experience.

If you have a new or small practice, take the unit to a health food store or shopping mall on the weekend and offer a free mini-session to shoppers.

## Muscle Testing (For Practitioners Only)

Muscle test patients prior to an *IonCleanse* session. Patients of medical doctors and chiropractors may have serious health problems and be extremely sensitive to electromagnetic fields or require a specialized format that can only be determined through muscle testing. First, determine if the patient is electrical, and then the appropriate session option as follows:

### To Determine If a Patient Is Electrical

1. Have the person hold an arm either straight out or off to the side (see video tape).
2. Instruct him/her to resist, and then apply gentle pressure to the arm just above the wrist. You should get a strong response virtually all of the time. If not, refer the patient to a chiropractor or physician.
3. Next, place your index finger on the bridge of the patient's nose and again instruct them to resist.
4. Test the arm again. The patient's arm should go weak and they should not be able to resist as they did on the initial try. If there is still strong resistance, the patient is not electrical and **must not be bathed**.
5. If the patient is electrical, go on to determine session option.

### To Determine the Program Setting

1. With the patient's feet in the water, turn the unit on, press start, then 7/mode, then 8/time to select Option 1 (All Positive).
2. Muscle test for positive polarity:
  - If the patient tests strong for positive, option 4 setting is suggested (15+/10-/5+).
  - If the patient tests weak for positive polarity, select Option 2 (negative (-) polarity).
3. Using All Negative (Option 2), muscle test for negative. If patient tests strong for negative, use option 5 (10-/15+/5-).

**Note:** If you are familiar with muscle testing, a shorter and simpler method is to muscle test while “asking” your patient which protocol they need. Be sure to muscle test throughout the session to verify that the setting is still right for the person. The vast majority of people require a varying ion field during the session. We have found that over a 30 minute session, a person will test strong to one ion field for a while, go weak in that field, test strong in the opposite ion field for a while, go weak in that field and test strong in the original field for the remainder of the session.

Because most practitioners have their own method of muscle testing, we suggest using whatever method you are most comfortable with.

Muscle testing may not work if your patient is dehydrated, highly stressed, or depleted of minerals. However, if they are on allopathic medications or have taken street drugs extensively in the past, and are not electrical, you should put them on a nutritional/supplement regimen for a month or so until they do test electrical.

## Nutritional Protocols

Cleansing the body accelerates catabolic and anabolic metabolism and requires extensive supplemental nutrition to maximize results. The liver, kidneys, lymph, adrenals and colon must be strengthened and supported to accommodate the increased stress placed upon them. Heavy metals dislodged from receptor sites during detoxification must be replaced by carbon-based minerals to prevent their being drawn back to those sites.

Everyone benefits from cleansing, but many people are too weak to plunge into a cleansing and purification program right away. The adrenal glands and organs of elimination of weak patients may need to be strengthened and supported for a few weeks prior to beginning a cleansing program.

## APEX Nutritionals

AMD is continually searching for food supplements and homeopathics to support the cleansing process. We have recently discovered Apex Energetics, a company that offers the most comprehensive line of support and regenerative products for cleansing and revitalization. Apex will sell to lay persons at retail prices and licensed practitioners at wholesale prices. For their product catalog, call toll-free (800)736-4381. In addition to the suggestions below, you may wish to include several of their other products in your ongoing program.

### General Cleansing Support

Many individuals are too weak or depleted to go into a cleansing and purification program immediately and should be nourished for 2-4 weeks with the following foods and homeopathics from Apex Energetics:

**Mineral-Zyme** – High quality mineral sources with digestive enzymes

**Master-Zyme** – Enzyme support for hypothalamus, pituitary and adrenals

**Super Digestzyme** – A powerful combination of digestive enzymes and herbs

**Glysen** – For individuals known to be insulin resistant


**Omegaco-3** or Super EFA Complex – Essential fatty acid supplement

**OxiCell** – Powerful antioxidant creams for reduction of oxidative stress. Oxidative stress indicates high levels of free radicals which are highly destructive ions resulting from errors in oxygen metabolism. These free radicals are present in abnormally high levels in energetically depleted and older persons, drug and alcohol addicts, people involved in competitive athletics and persons undergoing cleansing programs.

## Accelerating the Rejuvenation Process

For individuals interested in accelerating the rejuvenation process and for practitioners seeking to offer accelerated programs to their clients and patients, A Major Difference has discovered through the research efforts of a few practitioners that low-level laser stimulation of neurolymphatic reflex points can more than double the output of heavy metal debris in the bath water. The technique for accomplishing this is simple.

The chart below shows the neurolymphatic reflex points outlined in black. During the footbath, have the client move the probe of our 2-diode or 4-diode laser over the shaded areas in the front of the body for 2 minutes at a time. Repeat this process several times during the half hour footbath. **THIS PROCEDURE IS FOR ENERGETICALLY STRONG PERSONS ONLY.**

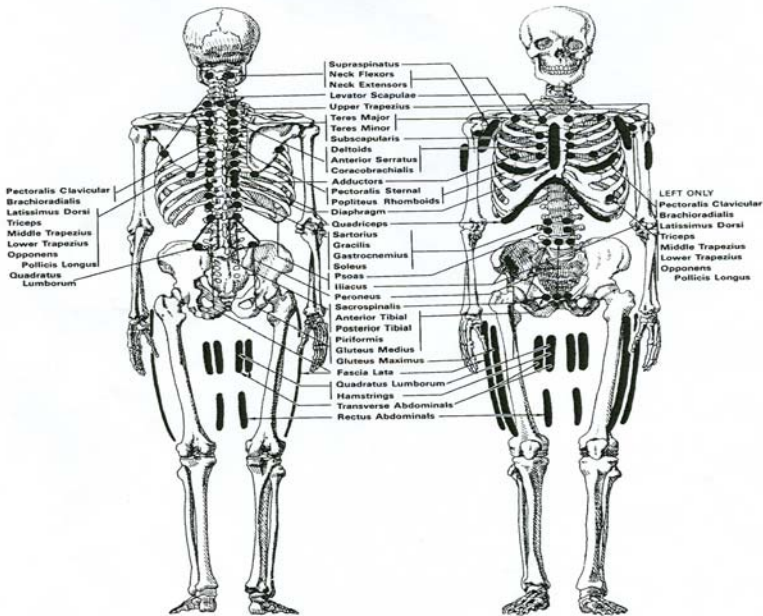

A Major Difference, Inc. manufactures a number of economically priced, FDA cleared, low-level hand held laser products that are ideal for this purpose. We especially recommend the Excalibur II and Excalibur IV lasers. Please call for pricing.

Low-level laser light has been shown to (1) increase cell utilization of oxygen, (2) increase cell production of ATP, the body's energy supply and (3) increase cell replication.

## Metal Plate Replacement


Your metal plate replacement kit contains:

1. Replacement metal plate assembly
2. Attachment hardware: main assembly (2½ inch bolt, copper spacer tube, wing-nut, washer) and wiring (2 rounded nuts)
3. Nut driver.


Note that the attachment kit includes new screws and nuts for wiring posts but these should not be necessary. If any hardware is missing, please call us.

### **Metal Plate Replacement Instructions**

1. With the unit standing vertically on a firm surface, use the red nut driver (supplied) to loosen and remove the two rounded nuts on top of array that attach the black and white wires.
2. Unscrew the wing-nut on back of array, and discard the nut and washer.
3. Withdraw the 2½ inch bolt to release copper tube and discard both.
4. Lay the unit on its back and pull off flat plastic front plate.
5. Remove old metal plate assembly.
6. Insert new metal plate assembly so that the three tabs fit into the three slots of the back panel.



7. Replace plastic front over new plate assembly so that the three tabs fit into the three slots of the front plate. Make sure the word “IonCleanse” is facing you and that the black terminal on top of the array is on the left, and the white terminal is on the right.
8. Holding the copper tube in place between the plastic panels, insert the long screw and tighten with the washer and wing-nut on the back.
9. Re-attach the electrical wires on top of the array, using the new replacement rounded top nuts, tightening with red nut-driver. Make sure you attach the black wire to the terminal marked “black” and the white wire to the terminal marked “white.”

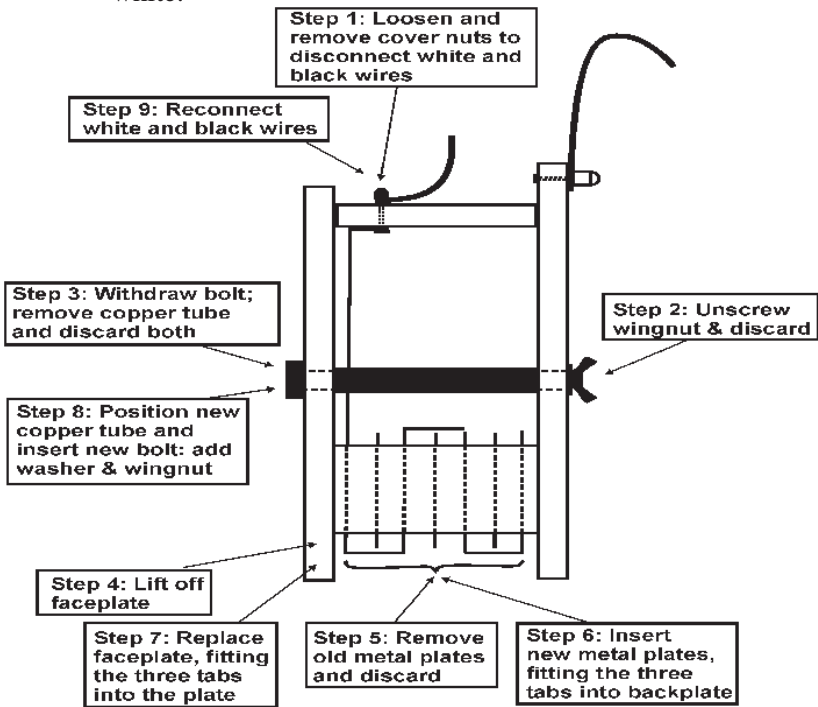

## Limited Warranty Information

The *IonCleanse* comes with a one-year limited warranty. A Major Difference, Inc. will repair the *IonCleanse* with new or rebuilt parts, free of charge, in the U.S.A. for one (1) year from the date of original purchase in the event of a defect in materials or workmanship.

This warranty only covers failures due to defects in materials or workmanship which occur during normal use. It does not cover damage which occurs in shipment; failures which are caused by products not supplied by A Major Difference, Inc.; or failures which result from accident, misuse, abuse, neglect, mishandling, misapplication, alteration or modification; service by anyone other than A Major Difference, Inc. or damage that is attributable to acts of God.

## Limits and Exclusions

There are no express warranties except as listed above. This warranty will be terminated if the seals located on the bottom of the unit are broken or the serial number on the back of the unit is altered, effaced, or removed. A Major Difference, Inc. shall not, in any case, be liable for medical expenses or special, incidental, or consequential damages caused by defects, failures, or malfunctions of any product, arising from breach of warranty, breach of contract, negligence, tort or any legal theory. All expressed and implied warranties, including the warranties of merchantability and fitness for a particular purpose, are limited to the applicable warranty period set forth above.

Some states do not allow the exclusion or limitation of incidental or consequential damages, or limitations on how long an implied warranty lasts, therefore some of the above exclusions or limitations may not apply to you.

This warranty gives you specific legal rights, and you may also have other rights, which vary from state to state.

## Two-Year Extended Warranty

A Major Difference, Inc. also offers a two-year extended limited warranty on each new unit purchased. You have up to one year from the original purchase date to buy this extended warranty. The same limits and exclusions from the standard warranty apply to the extended warranty. Please call us at 866-315-8638 to purchase the extended warranty.

## Array/Plate Replacement Log

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_

Date replaced: \_\_\_\_\_



2950 S. Jamaica Ct., Suite 300  
Aurora, CO 80014  
Phone: 303-755-0112  
Toll free: 877-315-8638  
Fax: 303-755-3022  
[www.amajordifference.com](http://www.amajordifference.com)